



OPTIONAL: You may find that a flip-top squirter lid is more practical for your application. The sprayer top that comes on the bottle can easily be replaced by unscrewing it and screwing the squirter lid on in its place.



ATTENTION

Please follow your physician's instructions on how to use this and any other product.



NOTE

The color of the universal Twin Compartment Bucket may be different than in the images shown.

QUESTIONS

For questions about this product...



Call us toll free at
(877) 717-5487



Visit us on the Web
www.ReBuilderMedical.com



Or email us at
help@ReBuildermedical.com



Warranty Information

All warranty claims are to be processed by the manufacturer directly and must be accompanied by a receipt or in your order history for proof of purchase.

FOR WARRANTY RELATED ISSUES PLEASE CALL BEFORE RETURNING TO REBUILDER® MEDICAL INC.

For questions concerning warranty, mechanical or operational problems with your ReBuilder® unit or accessories, please call toll free **877-717-5487**.

v210512

MADE IN USA



Universal Twin Compartment Bucket




ReBuilder Medical Inc.  304 - 725 - 4915
 304 - 725 - 2202
 636 Treeline Drive, Charles Town, WV 25414

To use the Twin-Compartment Footbath, you will need the following items:

- A. Universal Twin-Compartment Bucket
- B. ReBuilder® Electrolyte Spray
- C. Universal black non-adhesive pads
(These pads will attach to the lead wires on your ReBuilder® unit. - ReBuilder sold separately. See illustrations below.)



Find the "barrel" slot inserts on each non-adhesive pad for the lead wire.

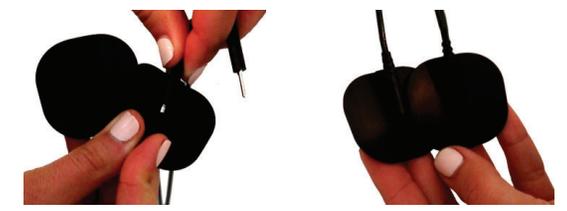

Slide the silver prong from your lead wire securely into each pad.

Using the Universal Twin-Compartment Bucket

..... 1
Add 1 teaspoon of electrolyte spray to each side of the Twin-compartment bucket.



..... 2
Fill the bucket with enough lukewarm water to reach your ankles when you place your feet into each side of the bucket.
(Less water can be used if desired.)



..... 3
Using the non-adhesive pads, attach them to your lead wire. Place one pad in each side of the bucket.
(The pads do not have to be touching your feet, just the water)



The pads will likely move around during the treatment. The pads transfer the signal to the water and the water transfers the signal to your feet.



If it is your first time using your ReBuilder stimulator, no matter which method you use for treatment, (bucket, conductive garments, or adhesive pads), make sure you follow the treatment guide found in your manual. If you have been using your unit previously with a different method and switching to this one, then you can continue to use your unit with the same time and intensity setting you would normally use.

Attach your lead wire to your ReBuilder stimulator. Turn the stimulator on to the appropriate setting *(see note above)*.



Sit back & relax while the device does the work and remain seated during the treatment. When your treatment session is finished, thoroughly dry your feet. Rinse and clean the bucket and also the non-adhesive pads to remove any skin debris, or oils, & to prevent a build-up of minerals.